

# Julabo Case Study

## JULABO PRESTO® A80

### Heating a 20 liters reactor from +50 °C to +100 °C



### Objective

This case study tests the heating power of JULABO PRESTO® A80 with a 20 liters glass reactor. The A80 is connected to the reactor via two 2.0 m metal tubings. The A80 is programmed to heat up from +50 °C to +100 °C.

### Test Conditions

JULABO unit	JULABO PRESTO® A80
Cooling power	+20 °C 1.2 kW
	0 °C 1.2 kW
	-20 °C 1.1 kW
Heating capacity	1.8 kW
Band limit	No
Flow pressure	0.40 bar
Bath fluid	JULABO Thermal HL80
Reactor	20 liters glass reactor (Asahi) filled with 18 liter JULABO Thermal HL80
Jacket volume	7.0 l
Control	External (ICC)

### Test Results

See chart on back page: The A80 heating process from +50 °C to +100 °C in 1h 40 min without overshoot.

### Environment

Room temperature	+20 °C
Humidity	45 %
Voltage	230 V / 50 Hz




### Tip

You can also use the robust Pt100 with PTFE coating.

More tips on back page >>



JULABO GmbH  
Eisenbahnstraße 45  
77960 Seelbach / Germany  
Tel. +49 (0) 7823 51-0

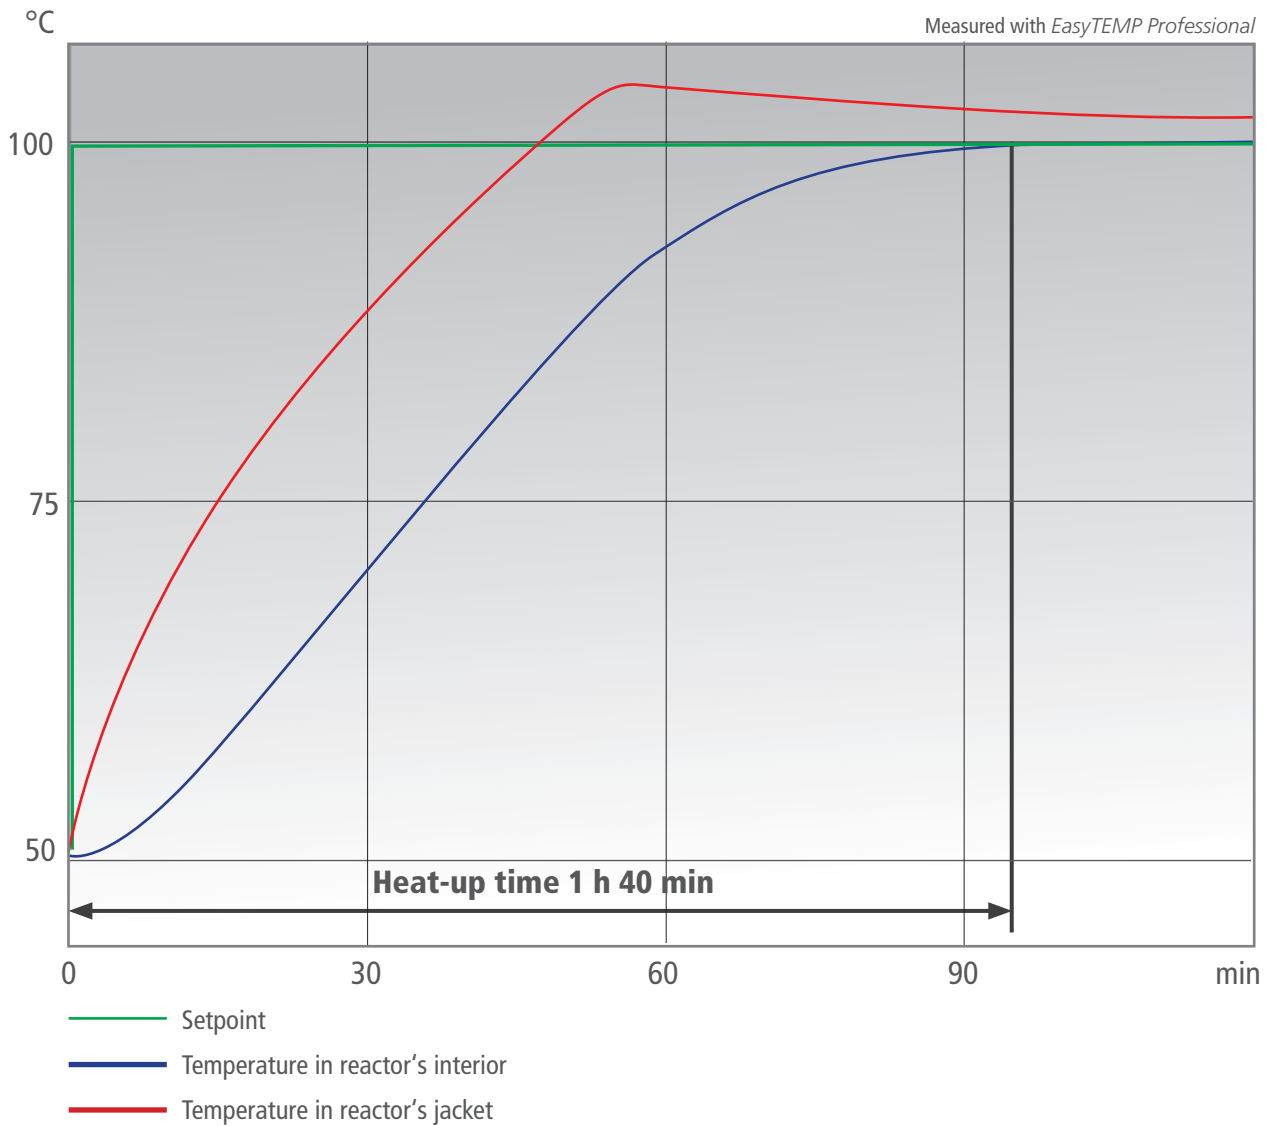

**Tip**

Make use of the option to regulate the pump pressure. You can define the desired pressure in the PRESTO® settings.



**Tip**

The Ethernet interface permits full access to all operational functions of the PRESTO®.



JULABO GmbH  
 Eisenbahnstraße 45  
 77960 Seelbach / Germany  
 Tel. +49 (0) 7823 51-0